

AnMa TECH

For all your bolting needs

| | |
|-------------|---------------------|
| Report nr.: | 36846528-05-20 |
| Serial nr.: | 152151850 |
| Tool: | FE055-3-230V-4 port |
| Ma min: | 0 |
| Ma max: | 700 |

| | |
|-------------|---------------------|
| Date: | 15-05-2020 |
| Technician: | André van Nijnatten |
| Equipment: | LEO2/700 Bar 8140 |

| Pressure (Bar) | Measured (Bar) | Difference % |
|----------------|----------------|--------------|
| 0 | 0 | 0 |
| 100 | 100 | 0,0 |
| 200 | 201 | 0,1 |
| 300 | 301 | 0,1 |
| 400 | 399 | -0,1 |
| 500 | 501 | 0,1 |
| 600 | 600 | 0,0 |
| 700 | 704 | 0,6 |

Result: Pressure gauge verified within 1% of full scale value


Signature: 

AnMa TECH

For all your bolting needs

| | |
|-------------------|------------|
| Calibration date: | 15-05-2020 |
| Calibration due: | 15-05-2021 |

| | |
|-------------|---------------------|
| Tool model: | FE055-3-230V-4 port |
| Serial nr.: | 152151850 |

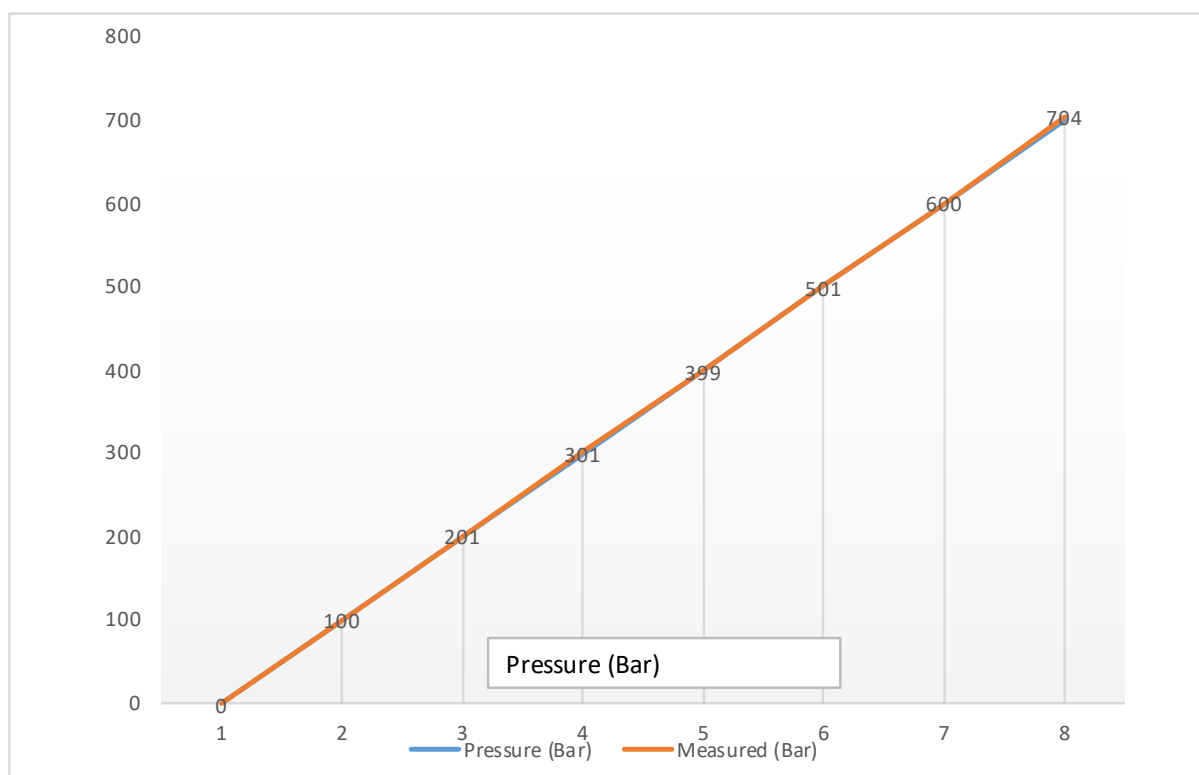

Disclaimer:

AnMa TECH BV does not take liability for any damage caused by observations made or remarks noted on this report.

Every check and/or test is a snap shot.

Performed following ISO/IEC 17025:2017

NEN 3140
KEURING

AnMa TECH
For all your bolting needs

Report nr.: 36846528-05-20 NEN3140
Serial nr.: 152151850
Tool: FE055-3-230V-4port

Date: 15-05-2020
Technician: André van Nijnatten
Equipment: EazyPat s/n 13H-0311

| TEST | RESULTAAT | MEETWAARDE | STATUS |
|------------------------------|-----------|-------------------|--------|
| Visuele controle | OK | nvt | GOED |
| Weerstandbeschermingsleiding | OK | 0,05 Ω | GOED |
| Isolatie weerstand | OK | >19,99 M Ω | GOED |
| Vervangende lekstroom | OK | 0,16mA | GOED |

| | | | |
|-----------|----|-----|------|
| RESULTAAT | OK | nvt | GOED |
|-----------|----|-----|------|

Result:

Signature:

