

AnMa TECH

For all your bolting needs

Report nr.:

36846805-0123

Serial nr.:

72112027

Tool:

FE055-3

Ma min:

0

Ma max:

700

Date:

24-01-2023

Technician:

Glenn van den Berg

Equipment:

LEO2/700 Bar 8140

Pressure (Bar)	Measured (Bar)	Difference %
0	0	0
100	101	0,1
200	201	0,1
300	301	0,1
400	398	-0,3
500	500	0,0
600	602	0,3
700	703	0,4

Result:

Pressure gauge verified within 1% of full scale value

Signature:




AnMa TECH

For all your bolting needs

Calibration date:	24-01-2023
Calibration due:	24-01-2024

Tool model:	FE055-3
Serial nr.:	72112027

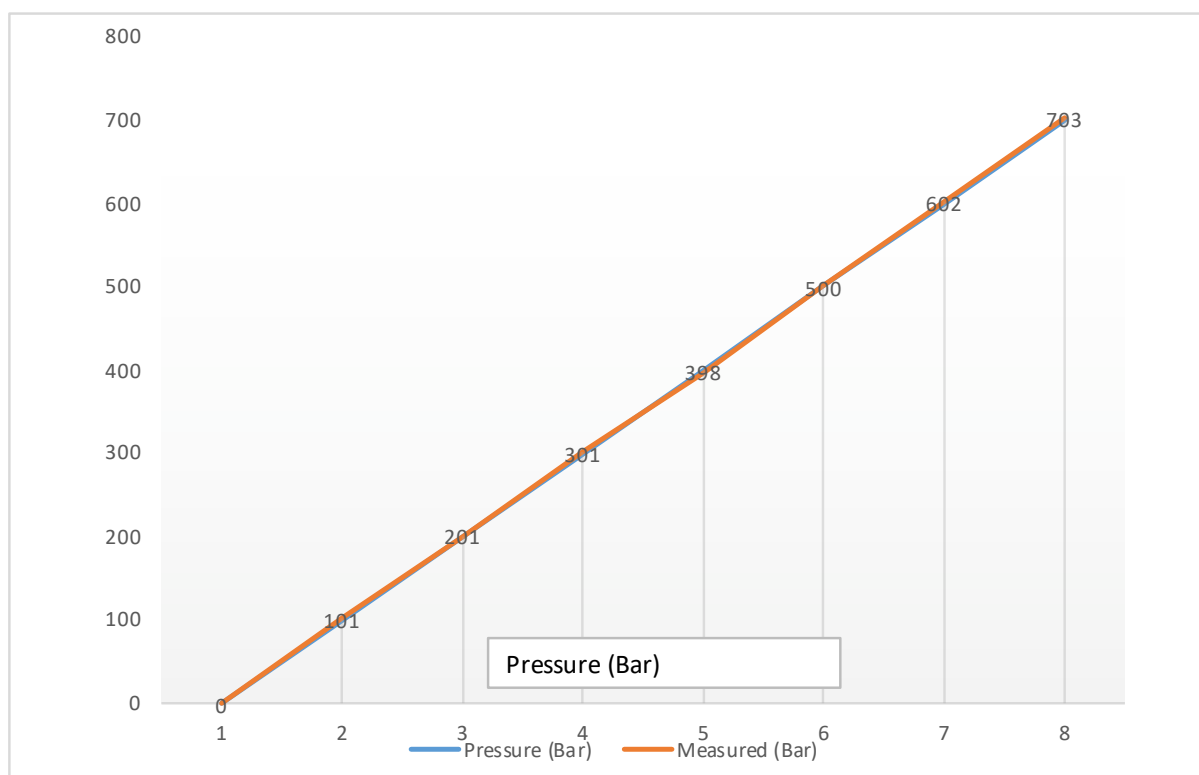

Disclaimer:

AnMa TECH BV does not take liability for any damage caused by observations made or remarks noted on this report.

Every check and/or test is a snap shot.

Performed following ISO/IEC 17025:2017

NEN 3140
KEURING

AnMa TECH
For all your bolting needs

Report nr.: 36846805-0123 NEN3140
Serial nr.: 72112027
Tool: FE055-3

Date: 24-01-2023
Technician: Glenn van den Berg
Equipment: EazyPat s/n 13H-0311

TEST	RESULTAAT	MEETWAARDE	STATUS
Visuele controle	OK	nvt	GOED
Weerstandbeschermingsleiding	OK	0,08 Ω	GOED
Isolatie weerstand	OK	>19,99 M Ω	GOED
Vervangende lekstroom	OK	0,20 mA	GOED

RESULTAAT	OK	NVT	GOED
-----------	----	-----	------

Result:



Signature: