

# AnMa TECH

*For all your bolting needs*

Report nr.:	36847505-0125
Serial nr.:	73810784
Tool:	<b>HDF2000G</b>
Ma min:	0
Ma max:	1500

Date:	01-01-2025
Technician:	Shiwanie Lalbahadoersing
Equipment:	LEO1/1500 Bar 1041

Pressure (Bar)	Measured (Bar)	Difference %
0	0	0
250	251	0,1
500	502	0,3
750	750	0,0
1000	1000	0,0
1250	1253	0,4
1500	1506	0,9

Result: **Pressure gauge verified within 1% of full scale value**


Signature: 

# AnMa TECH

*For all your bolting needs*

Calibration date:	01-01-2025
Calibration due:	01-01-2026

Tool model:	HDF2000G
Serial nr.:	73810784

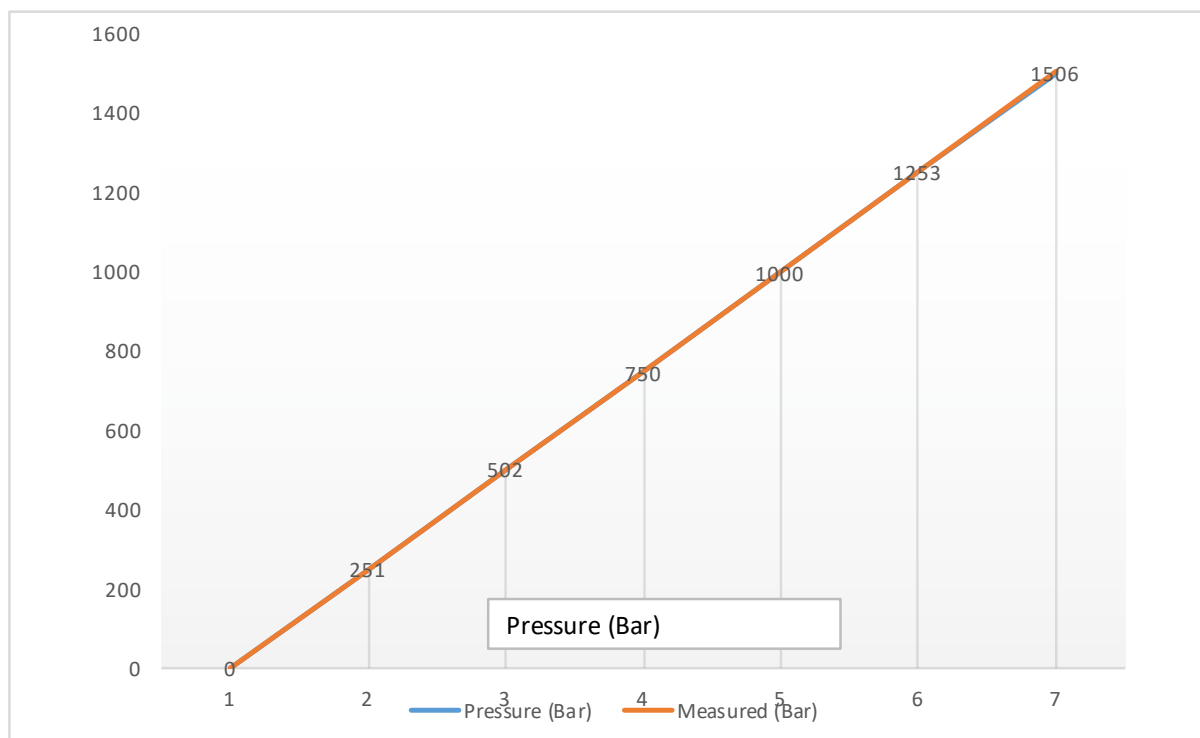

**Disclaimer:**

AnMa TECH BV does not take liability for any damage caused by observations made or remarks noted on this report.

Every check and/or test is a snap shot.