

# AnMa TECH

*For all your bolting needs*

Report nr.:	36847509-0125
Serial nr.:	72111155
Tool:	<b>FE055-3</b>
Ma min:	0
Ma max:	700

Date:	01-01-2025
Technician:	Shiwanie Lalbahadoersing
Equipment:	LEO2/700 Bar 8140

Pressure (Bar)	Measured (Bar)	Difference %
0	0	0
100	100	0,0
200	201	0,1
300	301	0,1
400	402	0,3
500	503	0,4
600	597	-0,4
700	699	-0,1

Result: **Pressure gauge verified within 1% of full scale value**


Signature: 

# AnMa TECH

*For all your bolting needs*

Calibration date:	01-01-2025
Calibration due:	01-01-2026

Tool model:	FE055-3
Serial nr.:	72111155

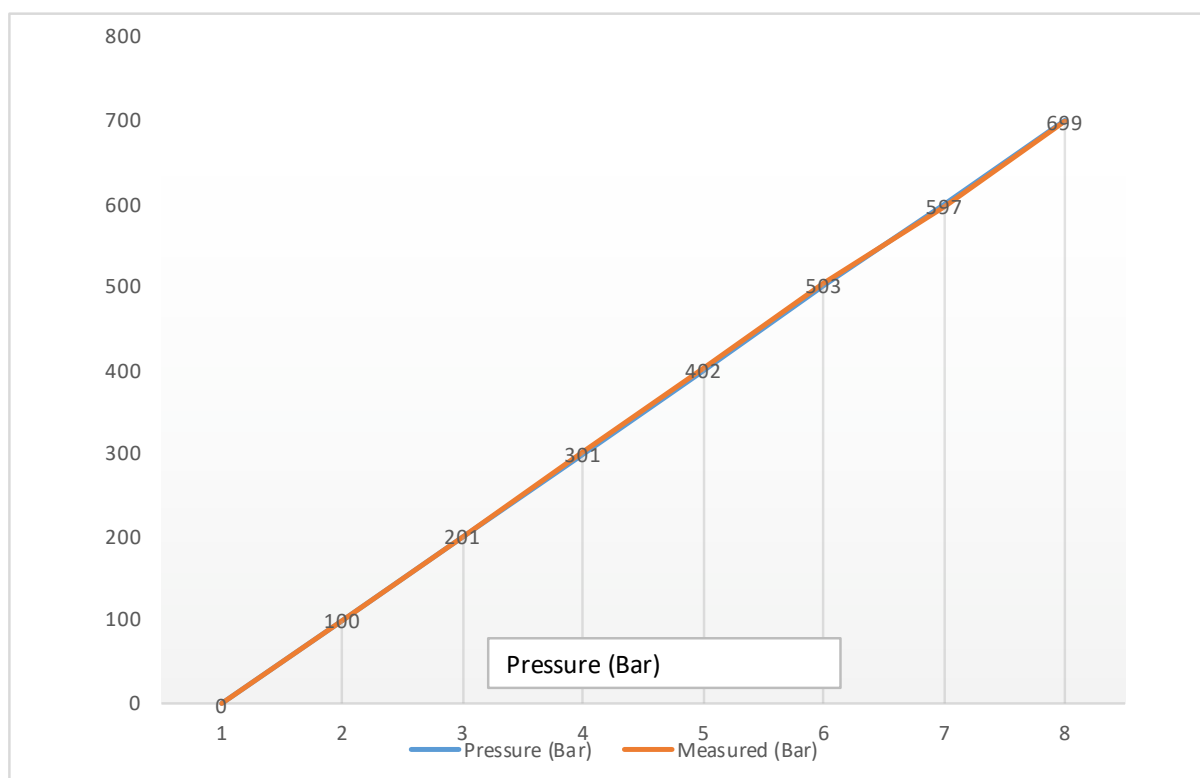

**Disclaimer:**

AnMa TECH BV does not take liability for any damage caused by observations made or remarks noted on this report.

Every check and/or test is a snap shot.

Performed following ISO/IEC 17025:2017

**NEN 3140**  
KEURING

# **AnMa TECH**

*For all your bolting needs*

Report nr.: 36847509-0125  
Serial nr.: 72111155  
Tool: FE055-3

Date: 01-01-2025  
Technician: Shiwanie Lalbahadoersing  
Equipment: EazyPat s/n 13H-0311

TEST	RESULTAAT	MEETWAARDE	STATUS
Visuele controle	OK	NVT	GOED
Weerstandbeschermingsleiding	OK	0,09 $\Omega$	GOED
Isolatie weerstand	OK	>19,99 M $\Omega$	GOED
Vervangende lekstroom	OK	0,19 mA	GOED

RESULTAAT	OK	NVT	GOED
-----------	----	-----	------

Result:



Signature: